




## Heat Shrink

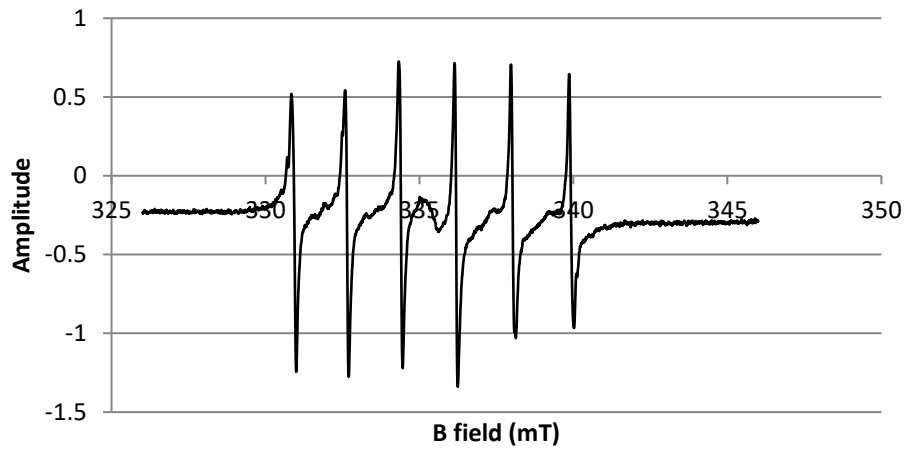


## Electrical Tape

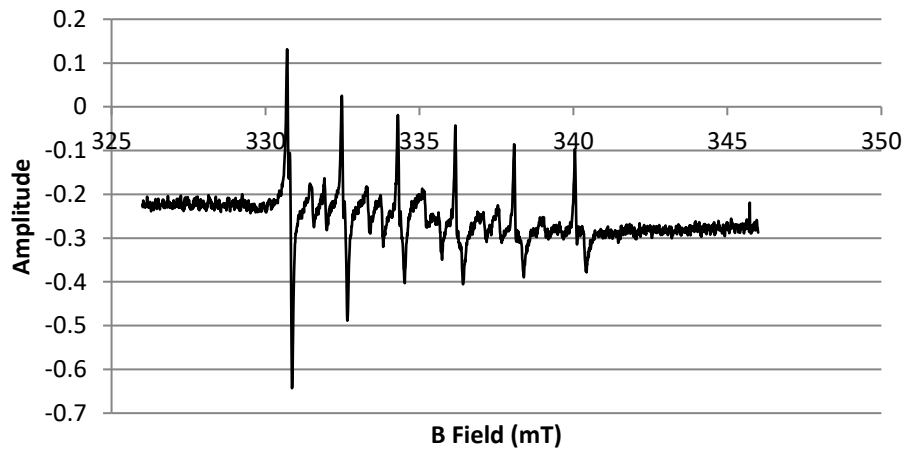


### Glass Tube Only

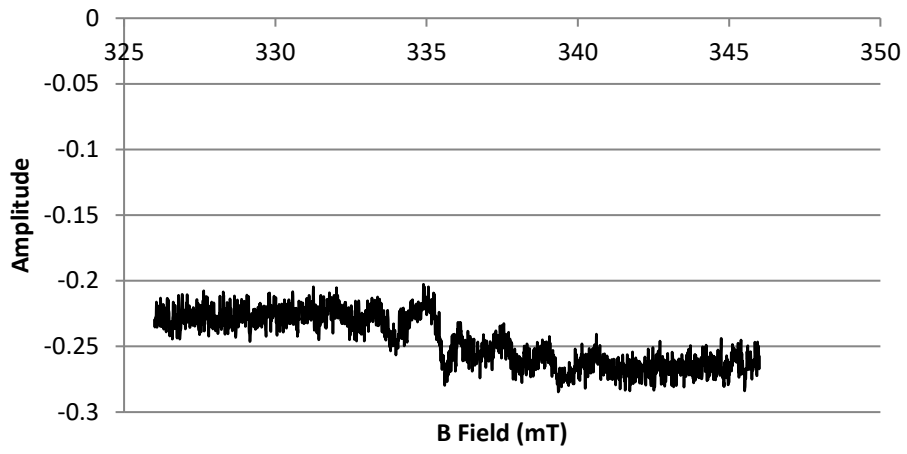


### Disposable Pipet

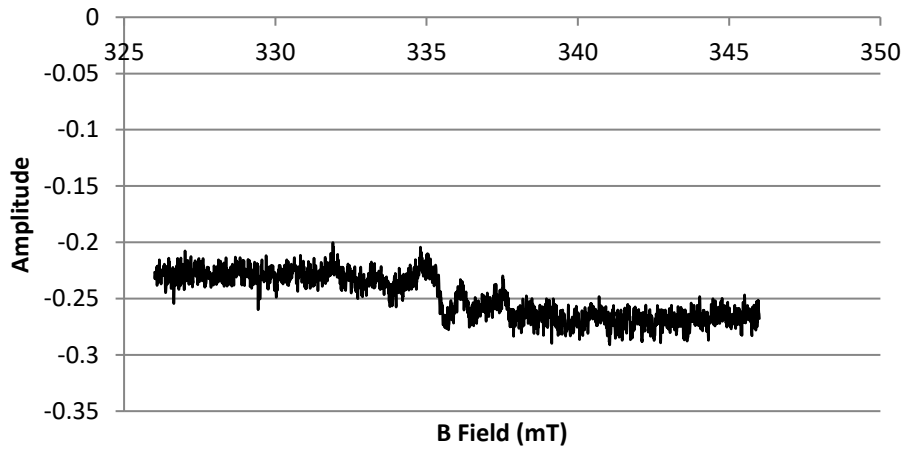


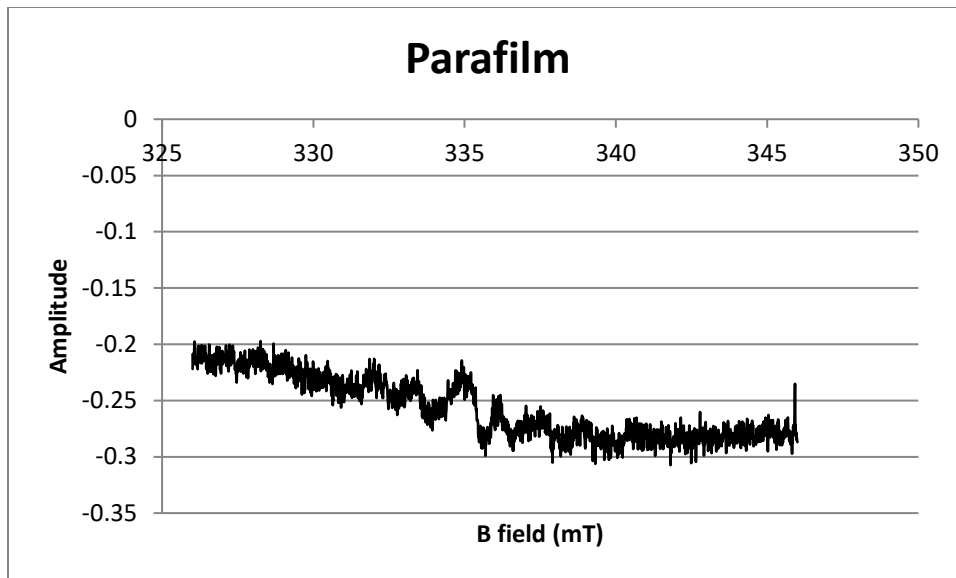


\*Parafilm was chosen to hold the tooth to the glass tube.

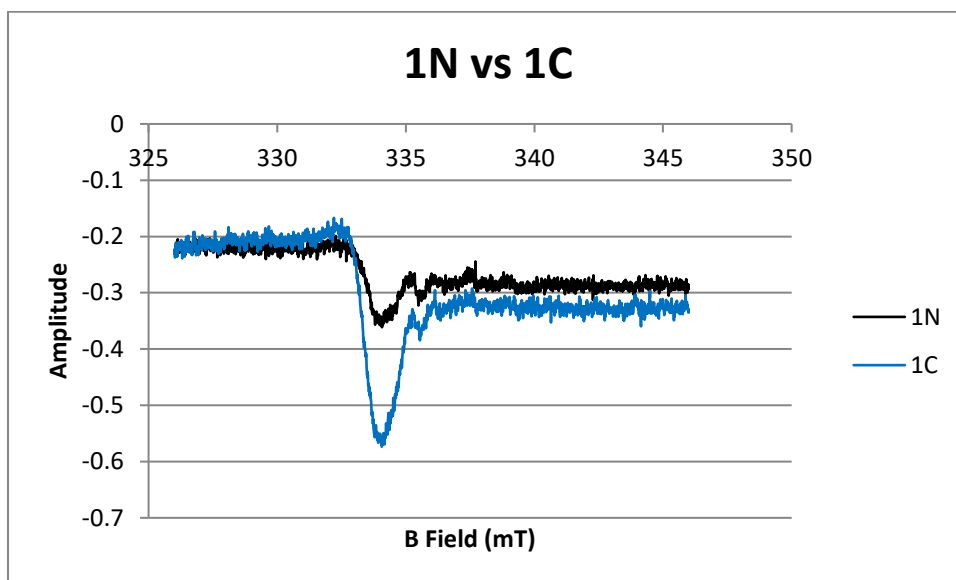


N denotes neutron irradiated half of tooth, C denotes control half of tooth

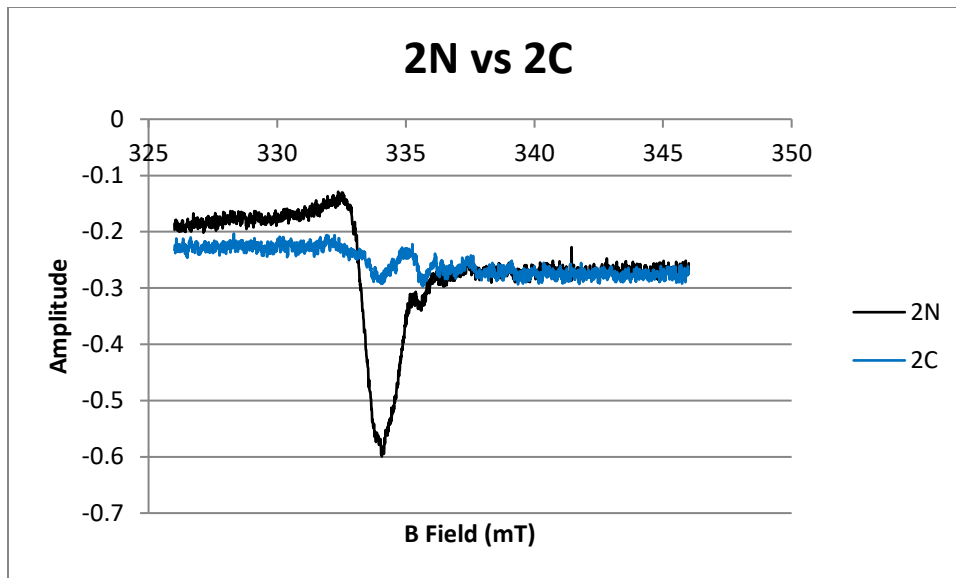

N denotes neutron irradiated half of tooth, C denotes control half of tooth

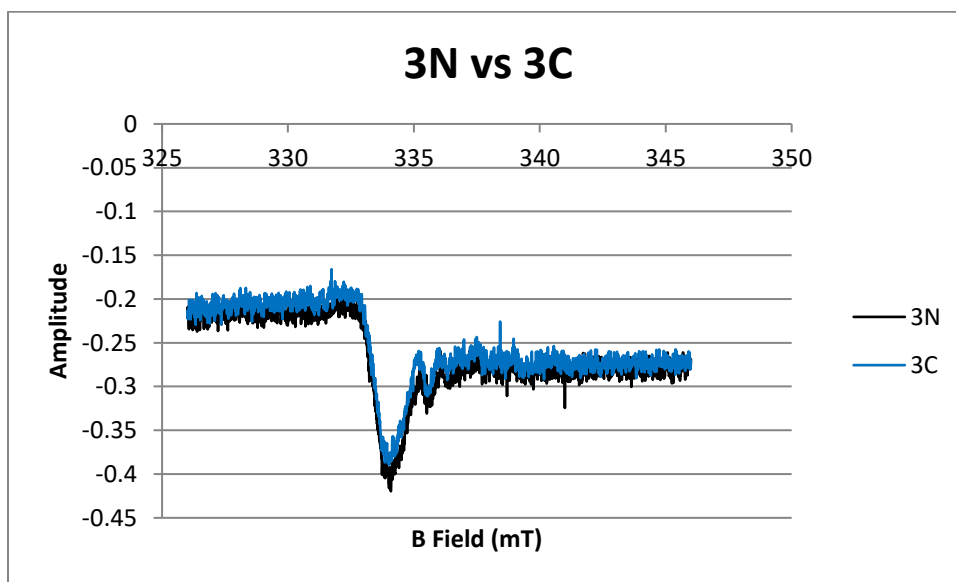

N denotes neutron irradiated half of tooth, C denotes control half of tooth

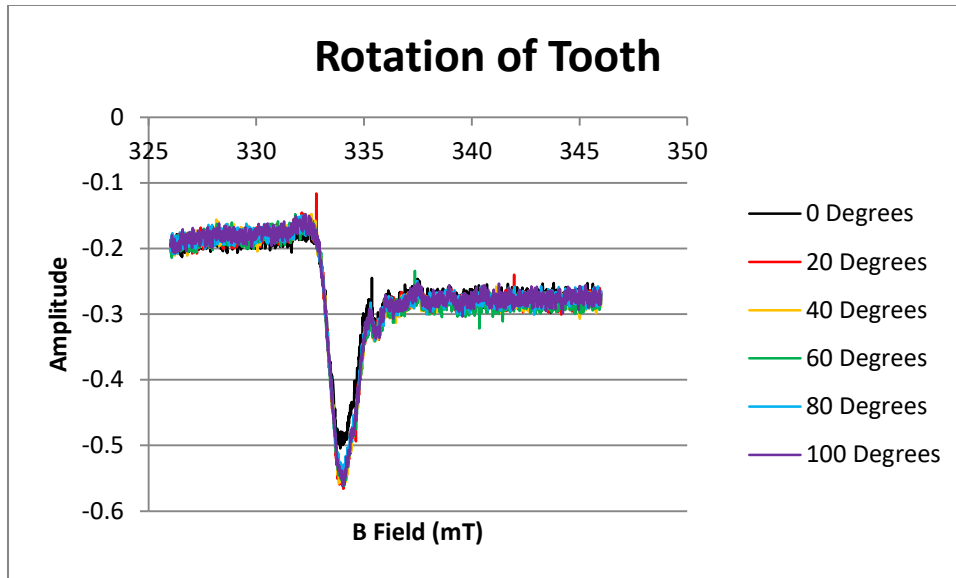

Tooth 1C rotated in 20 degree increments from 0-100 degrees.